

Antony Christy Catherine Mary¹, Susai Rajendran^{2,*},
Jayaprahasam Jeyasundari⁴, Rajendran Dorothy³

¹Parvathy's Arts and Science College, Department of Chemistry, Dindigul, Tamilnadu, India, Antony's College of Arts and Sciences For Women, ²Research center, Department of chemistry, Thamaripadi, Dindigul, Tamilnadu, India, ³AMET University, Kanathur, Chennai, India, ⁴SVN College, Department of Chemistry, Nagamalai, Madurai, Tamilnadu, India

Scientific paper

ISSN 0351-9465, E-ISSN 2466-2585

UDC:620.192.4:669.24.295

doi: 10.5937/ZasMat1704469C



Zastita Materijala 58 (4)
469 - 474 (2017)

Corrosion resistance of Ni-Ti alloy, SS18/8 alloy and thermoactive alloy in artificial saliva in the absence and presence of tea

ABSTRACT

Corrosion resistance of Ni-Ti alloy, SS18/8 alloy and thermoactive alloy in artificial saliva (AS) in the absence and presence of tea has been evaluated by such as polarization study. For Ni-Ti alloy, SS18/8 alloy and thermoactive alloy, polarization study lead to the conclusion that corrosion resistance of Ni-Ti alloy and thermoactive alloy decreases in the order

AS + Tea > Tea > AS

Hence, people implanted with orthodontic wire, made of Ni-Ti alloy and thermoactive alloy can take tea orally without any hesitation.

For SS18/8 alloy, polarization study lead to the conclusion that corrosion resistance of SS18/8 alloy decreases in the order

AS > AS + Tea > Tea

So, people implanted with orthodontic wire, made of SS18/8 alloy should avoid taking tea.

Keywords: corrosion resistance, orthodontic wires, artificial saliva, extract tea, Ni-Ti alloy, SS18/8 alloy, thermoactive alloy, polarization study.

1. INTRODUCTION

Corrosion is the one of the most common process. It is a natural, spontaneous and thermodynamically favorable process. This problem caused by the defects in the components of the implants. Corrosion is destruction of materials when they interact with the the environment. The teeth could be regularized and by using orthodontic wires. Orthodontic wires can be made of many metals and alloys. After implantation many food items, many tablets are also orally taken. In the oral environment these orthodontic wires undergo many types of corrosion. In dentistry, metallic materials are used as implants in reconstructive oral surgery to replace a single tooth or an array of teeth [1]. Many metals and alloys have been used in dentistry. The corrosion behavior in artificial saliva has been investigated. The effect of different concentrations of eugenol in artificial saliva on titanium corrosion has been investigated by Kinani

and Chtaini [2]. Corrosion resistance tests of the CrNi, NiTi, and CuNiTi wires showed comparable data of parameters obtained in artificial saliva. The effects of multilayered Ti/TiN or single-layered TiN films deposited by pulse-biased arc ion plating (PBAIP) on the corrosion behavior of NiTi orthodontic brackets in artificial saliva have been investigated by Liu et al. [3]. The corrosion resistance of stainless steel 316L, mild steel (MS), and mild steel coated with zinc (MS-Zn) has been evaluated in artificial saliva in the absence and presence of spirulina, D-Glucose and electrol[4]. Five non-precious Ni-Co based alloys have been analyzed with respect to their corrosion behavior in artificial saliva [5]. The corrosion resistance of orthodontic wire made of 18 carat gold, in artificial saliva in presence of a tablet Brufen 400 mg has been investigated by MohamedKasim sheit et al., The corrosion behavior of palladium silver binary alloy, TiCrNi, NiTi, CuNiTi, dental amalgam [6-11], in artificial saliva has been investigated. Corrosion resistance of two orthodontic wires made of thermoactive superelastic shape memory alloy and 22 K gold in artificial saliva in the absence and presence of syzygium cumini extract has been evaluated by Madhumitha et al.[12]. Corrosion resistance of Super Elastic Nickel-Titanium alloy in

*Corresponding author: Susai Rajendran

Email: susairajendran@gmail.com

Paper received: 21. 07. 2017.

Paper corrected: 07.09.2017.

Paper accepted: 12.09.2017.

Paper is available on the website:

www.idk.org.rs/journal

artificial saliva, in the absence and presence of a tablet namely, Almox 250mg has been evaluated by Rajendran et al. [13 - 20]. Various metals and alloys have been used as biomaterials whose corrosion resistance has been investigated in artificial body fluids; various metals and alloys such as Ni-Al-Fe intermetallic alloys [21], titanium alloy [22], NiTi alloy [23], CoCrMo alloys [24,25], magnesium alloy [26,27], Cr-Ni stainless steel, Cr-Ni-Mo stainless steel [28], 316L stainless steel [29-31]. Corrosion inhibiting properties of some crown ethers on corrosion of stainless steel (types 304 and 316) in hydrochloric acid has been evaluated by Abdallah et al., [32]. Corrosion behaviour of SS 316 L in artificial saliva in presence of electrolite has been studied by Rajendran et al. [33]. Christy et al., have studied that the Influence of corrosion resistance of orthodontic wires in artificial saliva in the absence and presence of coffee [34].

2. EXPERIMENTAL

Orthodontic wires made of Ni/Ti, SS 18/8 and thermoactive alloys were used in the present study. The alloys were used as working electrode. Corrosion behavior of Ni/Ti, SS 18/8 and thermoactive alloys have been investigated in various test solution such as Artificial Saliva, Tea, Artificial Saliva +Tea. Orthodontic wires immersed in Fusayamma Meyer artificial saliva whose composition is

Table 1: Composition of Artificial Saliva

Tabela 1. Sastav veštačke pljuvačke

S.No	Name of the chemicals	Weight/lit
1	KCl	0.4g/l
2	NaCl	0.4g/l
3	NaH ₂ PO ₄ ·2H ₂ O	0.690g/l
4	Urea	1g/l
5	CaCl ₂ ·H ₂ O	0.906g/l
6	Na ₂ S·9H ₂ O	0.005g/l

3. RESULT AND DISCUSSION

3.1. Potentiodynamic Polarization study

Polarization analysis has been used for detection of the protective film formation on the metal surface during corrosion inhibition process. Polarization studies were carried out in a CHI-Electrochemical workstation with impedance,

Model 660A. A three-electrode cell assembly was used. The working electrode was one of the three alloys. A saturated calomel electrode (SCE) was the reference electrode while platinum was the counter electrode. From the polarization study, corrosion parameters such as corrosion potential (E_{corr}), corrosion current (I_{corr}), and Tafel Slopes (anodic = b_a and cathodic = b_c) were calculated.

3.2. Analysis of Polarization curves

Corrosion resistance of Ni-Ti alloy, SS18/8 alloy and thermoactive alloy in various test solutions has been evaluated by polarization study. When corrosion resistance increases Linear Polarization Resistance (LPR) increases; corrosion current (I_{corr}) decreases [33-41].

Ni – Ti alloy

The polarization curves of Ni-Ti alloy immersed in various test solutions are shown in Fig 1. The corrosion parameters namely Corrosion Potential (E_{corr}), Tafel slopes (b_c = cathodic; b_a =anodic), Linear Polarization Resistance (LPR) and Corrosion current (I_{corr}) are given in Table 2.

When Ni-Ti alloy is immersed in Artificial Saliva (AS), Linear Polarization Resistance (LPR) value is 3277970 ohm cm². The Corrosion current (I_{corr}) is 1.488×10^{-8} A/ cm². The Corrosion Potential (E_{corr}) is -375 mV vs SCE. When Ni-Ti alloy immersed in Tea, Linear Polarization Resistance (LPR) value increases from 3277970 to 3422320 ohm cm². The Corrosion current (I_{corr}) decreases from 1.488×10^{-8} to 1.300×10^{-7} A/ cm². This indicates that Ni-Ti alloy is more corrosion resistant in Tea. Further, the Corrosion Potential (E_{corr}) value shifts from -375 to -553 mV vs SCE. A protective film is forms on the metal surface. When Ni-Ti alloy immersed in the system consisting of AS and Tea, the LPR value further increases to 4697814 ohm cm². The Corrosion Current decreases to 8.420×10^{-9} A/ cm². This indicates that Ni-Ti alloy is more corrosion resistant in AS + Tea system than in Tea system or AS system. Further, the Corrosion Potential shifts to -638 mV vs SCE. Thus the polarization study leads to the conclusion that when Ni-Ti alloy is immersed in various test solution, the decreasing order of corrosion resistance of Ni-Ti alloy is as follows:

$$AS + Tea > Tea > AS$$

This study reveals that people having orthodontic wires made of Ni-Ti alloy should not hesitate to take Tea. The reason for it is because in this medium the corrosion resistance of Ni-Ti alloy increases.

Table 2: Corrosion parameters of alloys immersed in Artificial Saliva (AS) in the presence and absence of Tea, obtained by Polarization study

Tabela 2. Parametri korozije legura uronjenih u veštačku plivačku (AS) u prisustvu i odsustvu čaja, dobijeni polarizacionim ispitivanjima

Metal	System	E_{corr}	b_c	b_a	LPR	I_{corr}
		mVvs SCE	mV/decade	mV/decade	Ohm cm ²	A/cm ²
Ni-Ti alloy	AS	-375	178	302	3277970	1.488x10 ⁻⁸
	Tea	-553	143	359	342232	1.300x10 ⁻⁷
	AS+ Tea	-638	129	310	4697814	8.420x10 ⁻⁹
SS 18/8	AS	-343	193	302	2638460	1.942x10 ⁻⁸
	Tea	-391	176	273	2101240	2.210x10 ⁻⁸
	AS+ Tea	-657	162	296	964243	4.717x10 ⁻⁸
Thermoactive	AS	-501	158	315	7636745	5.775x10 ⁻⁹
	Tea	-466	171	212	14251401	2.767x10 ⁻⁹
	AS+ Tea	-622	142	280	8369940	4.890x10 ⁻⁹

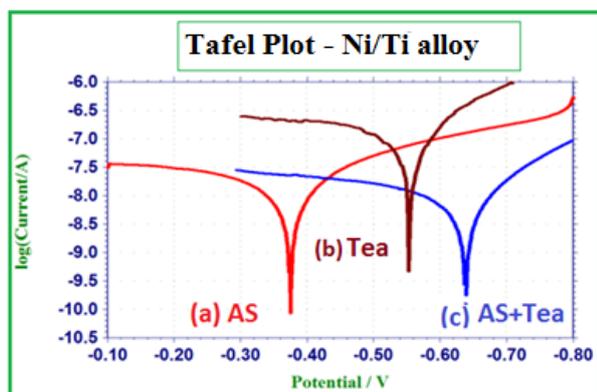


Figure 1. Polarization curve of Ni-Ti alloy immersed in various test solution: (a) AS (b) Tea (c) AS + Tea

Slika 1. Polarizacione krive legure Ni-Ti uronjene u različite ispitivane rastvore: (a) AS (b) Čaj (c) AS + Čaj

3.3. SS18/8 alloy

The polarization curves of SS18/8L alloy immersed in various test solutions are shown in Fig 2. The corrosion parameters namely Corrosion Potential (E_{corr}), Tafel slopes (b_c = cathodic; b_a =anodic), Linear Polarization Resistance (LPR)

and Corrosion current (I_{corr}) are given in Table 2. When SS18/8 alloy immersed in Artificial Saliva (AS), Linear Polarization Resistance (LPR) value is 2638460 ohm cm². The Corrosion current (I_{corr}) is 1.942 x10⁻⁸ A/ cm². The Corrosion Potential (E_{corr}) is -343 mV vs SCE. When SS18/8 alloy immersed in Tea, Linear Polarization Resistance (LPR) value decreases to 2101240 ohm cm². The Corrosion Current (I_{corr}) increases to 2.210 x10⁻⁸A/ cm². This indicates that corrosion resistant of SS18/8 alloy decreases in Tea, when compare to the one in saliva system. When SS18/8 alloy is immersed in AS and Tea system, the LPR value further decreases (964243 ohm cm²) while the corrosion current value (4.717 x10⁻⁸A/ cm²) further increases. This indicates the corrosion resistance of SS18/8 alloy decreases in AS + Tea system. Thus the polarization study leads to the conclusion that when SS18/8 alloy is immersed in various test solutions, the decreasing order of corrosion resistance of SS18/8 is as follows:

$$AS > Tea > AS + Tea$$

This study suggests that people having orthodontic wires made of SS18/8 alloy should avoid taking Tea. The reason for it is because in this medium the corrosion resistance of SS18/8 alloy decreases.

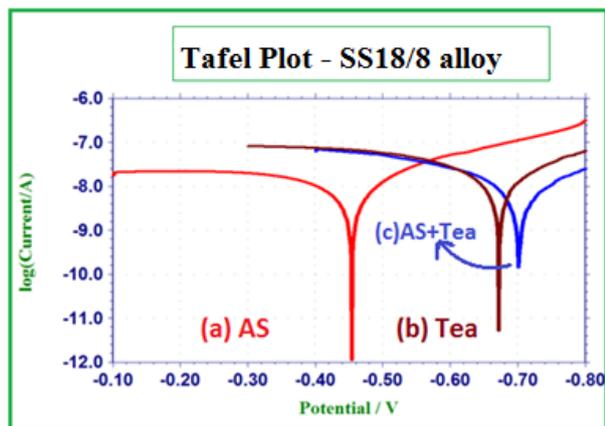


Figure 2. Polarization curve of SS18/8 alloy immersed in various test solution: (a) AS (b) Tea (c) AS + Tea

Slika 2. Polarizacione krive legure SS18/8 uronjene u različite ispitivane rastvore: (a) AS (b) Čaj (c) AS + Čaj

3.4. Thermoactive alloy

The polarization curves of Thermoactive alloy immersed in various test solutions are shown in Fig 3. The corrosion parameters namely Corrosion Potential (E_{corr}), Tafel slopes (b_c = cathodic; b_a =anodic), Linear Polarization Resistance (LPR) and Corrosion current (I_{corr}) are given in Table 2.

When Thermoactive alloy immersed in Artificial Saliva (AS), Linear Polarization Resistance (LPR) value is 7936745 ohm cm^2 . The Corrosion current (I_{corr}) is 5.775×10^{-9} A/ cm^2 . The Corrosion Potential (E_{corr}) is -501 mV vs SCE. When Thermoactive alloy immersed in Tea, Linear Polarization Resistance (LPR) value increases from 7936745 to 14251401 ohm cm^2 . The Corrosion current (I_{corr}) decreases to 2.767×10^{-9} A/ cm^2 . This indicates that Thermoactive alloy is more corrosion resistant in Tea. Further the Corrosion Potential (E_{corr}) value is -466 mV vs SCE. A protective film forms on the metal surface. When Thermoactive alloy immersed in the system consisting of AS and Tea, the LPR value further increases to 8369940 ohm cm^2 . The corrosion current decreases to 4.890×10^{-9} A/ cm^2 than in AS system. This indicates that Thermoactive alloy is more corrosion resistant in AS + Tea system than in Tea system or AS system. Further, the corrosion potential shifts to -622 mV vs SCE. Thus, the polarization study leads to the conclusion that when Thermoactive alloy is immersed in various test solutions, the decreasing order of corrosion resistance of Thermoactive alloy is as follows:

$$AS + Tea > Tea > AS$$

This study reveals that people having orthodontic wires made of Thermoactive alloy

should not hesitate to take Tea. The reason for it is because in this medium the corrosion resistance of Thermoactive alloy increases.

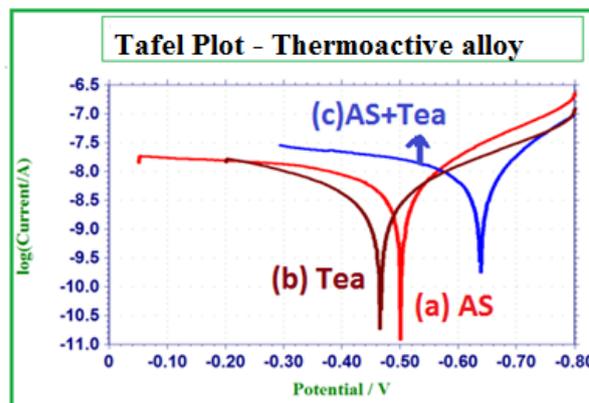


Figure 3. Polarization curve of Thermoactive alloy immersed in various test solution: (a) AS (b) Tea (c) AS + Tea

Slika 3. Polarizacione krive Termoaktivne legure uronjene u različite ispitivane rastvore: (a) AS (b) Čaj (c) AS + Čaj

4. CONCLUSION

- Corrosion resistance of Ni-Ti alloy, SS18/8 alloy and Thermoactive alloy in artificial saliva (AS) in the absence and presence of Tea has been evaluated by polarization study.
- For Ni-Ti alloy and Thermoactive alloy polarization study leads to the conclusion that corrosion resistance of Ni-Ti alloy and Thermoactive alloy decreases in the order
 - AS + Tea > Tea > AS
- For SS316L alloy polarization study leads to the conclusion that corrosion resistance of SS18/8 alloy decreases in the order
 - AS > Tea > AS + Tea
- People implanted with orthodontic wire, made of Ni-Ti alloy and Thermoactive alloy can take Tea orally without any hesitation.
- People implanted with orthodontic wire, made of SS18/8 alloy should avoid taking Tea orally.

Acknowledgment

The authors are thankful to their respective managements, for their constant help and encouragement.

REFERENCES

- [1] H.Mohamed Kasim Sheit, M.Seeni Mubarak, S.S.Syed Abuthahir, S.Rajendran (2017) Corrosion behaviour of 18 carat goldwith artificial saliva in presence of brufen 400mg tablet, Int.J.Nano Corros.Sci and Engg, 4(1), 58-66.

- [2] L. Kinani, A.Chtaini (2007) Corrosion Inhibition of Titanium in Artificial Saliva Containing Fluoride, *Leonardo Journal of Sciences*, 11, 3340-3348.
- [3] L.Chenglong, K.Paul Chu, L.Guoqiang, D.Yang (2007) Effects of Ti/TiN Multilayer on Corrosion Resistance of Nickel-Titanium Orthodontic Brackets in Artificial Saliva, *Corrosion Science*, 49, 3783–3796.
- [4] S.Rajendran, J.Paulraj, P.Rengan, J.Jeyasundari, M.Manivannan (2009) Corrosion Behavior of Metals in Artificial Saliva in Presence of Spirulina Powder, *Journal of Dentistry and Oral Hygiene*, 1, 1–8.
- [5] D.Mareci, Gh.Nemtoi, N.Aelenei, C.Bocanu (2005) The Electrochemical Behavior of Various Non-Precious Ni and Co Based Alloys in Artificial Saliva, *European Cells and Materials*, 10, 1–7.
- [6] L.Joska, M.Marek, J.Leitner (2005) The Mechanism of Corrosion of Palladium–Silver Binary Alloys in Artificial Saliva, *Biomaterials*, 26, 1605–1611.
- [7] M.A.Christopher Brett, Florin Trandafir (2004) The Corrosion of Dental Amalgam in Artificial Salivas: An Electrochemical Impedance Study, *Journal of Electro analytical Chemistry*, 52, 347–354.
- [8] M.A.Christoper Brett, I.Ioanitescu, F.Trandafir (2004) Influence of the Biological Fluid on the Corrosion of Dental Amalgam, *Corrosion Science*, 46, 2803–2816.
- [9] V.Raman, S.Tamilselvi, S.Nanjundan, N.Rajendran (2005) Electrochemical Behavior of Titanium and Titanium Alloy in Artificial Saliva, *Trends Biomater. Artif.Organs*, 18,137–140.
- [10] A.Ziebowicz, W.Walke, A.Barucha-Kepka, M.Kiel (2008) Corrosion Behavior of Metallic Biomaterials Used as Orthodontic Wires, *Journal of Achievements in Materials and Manufacturing Engineering*, 27, 151–154.
- [11] K.Fumiyo, O.Keiji, TKiyoko (1998) Surface Corrosion of Precious Dental Alloys Caused by Compound Iodine Glycerin in Artificial Saliva, *Electrochimica Acta*, 43, 1873–1879.
- [12] S.Madhumitha, V.Priyadharshini, A.Sheela, C.Aadhithya, M.Sangeetha, S.Rajendran (2016) Can people implanted with orthodontic wires made of thermoactive superelastic shape memory alloy and 22 k gold take syzygium cumini fruit juice orally?, *Int.J.NanoCorros.Sci and Engg.*, 3(4), 80 - 87.
- [13] CA.Loto, A.I.Mohammed (2003) Inhibition evaluation of mango juice extracts on the corrosion of mild steel in HCl, *Corrosion Prevention and Control*, 50(3), 107-118.
- [14] C.A.Loto, A.I.Mohammed (2000) The effect of cashew juice extract on corrosion inhibition of mild steel in HCl, *Corrosion Prevention and Control*, 47(2), 50-56.
- [15] J.C.Da Rocha, J.A.da Cunha Ponciano Gomes, E.D.Elia (2010) Corrosion inhibition of carbon steel in hydrochloric acid solution by fruit peel aqueous extracts, *Corrosion Science*, 52(7), 2341-2348.
- [16] P.C.Okafor, E.E.Ebenso (2007) Inhibitive action of Carica papaya extracts on the corrosion of mild steel in acidic media and their adsorption characteristics, *Pigment and Resin Technology*, 36(3), 134-140.
- [17] S.L.Priya, A.Chitra, S.Rajenderan, K.Anuradha (2005) Corrosion behaviour of aluminium in rain water containing garlic extract, *Surface Engineering*, 21(3), 229-231.
- [18] A.Bouyanzer, B.Hammouti (2004) Naturally occurring ginger as corrosion inhibitor for steel in molar hydrochloric acid at 353 K, *Bulletin of Electrochemistry*, 20(2), 63-65.
- [19] A.Singh, M.A.Quraishi (2015) The extract of Jamun (*Syzygiumcumini*) seed as green corrosion inhibitor for acid media, *Research on Chemical Intermediates*, 41 (3), 2901–2914
- [20] S.Rajendran, A.Krishnaveni, G.Muthukumar (2016) Corrosion Resistance Of Super Elastic Nickel - Titanium Alloy In Artificial Saliva In Presence Of Almox 250mg Tablet , *Int J Nano Corr Sci and Engg*, 3(4), 254-266.
- [21] I.E.Castaneda, J.G.Gonzalez-Rodriguez, J.Colin, M.A.Neri-Flores, I.E.Castaneda, J.G. Gonzalez-Rodriguez, J.Colin, M.A.Neri-Flores (2010) Electrochemical behavior of Ni-Al-Fe alloys in simulated human body solution, *J. Solid State Electrochem*, 14(7),1145-1152.
- [22] W.Zhou, T.Shen, N.N.Aung (2010) Effect of heat treatment on corrosion behaviour of magnesium alloy AZ91D in simulated body fluid, *Corros. Sci.* , 52(3),1035-1042.
- [23] A.K.Shukla, R.Balasubramaniam (2006) Effect of surface treatment on electrochemical behavior of CP Ti, Ti–6Al–4V and Ti–13Nb–13Zr alloys in simulated human body fluid, *Corros. Sci*, 48(7),1696-1703.
- [24] D.Sun, J. A.Wharton, R. J. K.Wood (2009) Abrasive size and concentration effects on the tribo-corrosion of cast CoCrMo alloy in simulated body fluids, *Tribology Int.*, 42(11), 1595-1604.
- [25] D.Sun, J.A.Wharton, R.J.K.Wood, L.Ma, W.M.Rainforth (2009) Microabrasion–corrosion of cast CoCrMo alloy in simulated body fluids, *Tribology Int.*, 42(1),99-107.
- [26] M.Daniel, A.Cailean, G. Bolat, I.Crețescu, D. Sutiman (2009) Comparative corrosion study of Ag-Pd and Co-Cr alloys used in dental applications, *Stud.Univ. Babeş-Bolyai. Chem.*, 1, 93-101.
- [27] Y.Song, D. Shan, R.Chen, F.Zhang, E.-H.Han (2009) Biodegradable behaviors of AZ31 magnesium alloy in simulated body fluid, *Mater.Sci.Eng C*, 29(3), 1039-1046.
- [28] B.Tutunaru, A. P.Samide, M.Preda (2007) Study of 316L stainless steel corrosion in cvasibiological conditions, *Rev. Chim*, 58(10),923-932.
- [29] R. W.-W.Hsu, C.-C. Yang, C.-A.Huang, Y.-S.Chen (2004) Investigation on the corrosion behavior of Ti–6Al–4V implant alloy by electrochemical techniques, *Mater.Chem. Phys*, 86(2), 269-276.
- [30] P.Peng, S.Kumar, N.H.Voelcker, E.Szili, R.Smart, St.C.,Griesser, H.J.J.Biomed (2006) Thin calcium phosphate coatings on titanium by electrochemical deposition in modified simulated body fluid, *Mater. Res - Part A*, 76 (2), 347-355.

- [31] A.S.Fouda, W.M.Abo-Elmeaty, H.M.El Abbasy (2010) Corrosion inhibition of aluminum-silicon alloy in H_2SO_4 solution using some thiophene derivatives, *Zastita Materijala*, 51(3), 133-143.
- [32] M. Abdallah, A. S. Fouda S. M. El-Ashrey (2011) Amino acids as environmentally-friendly corrosion inhibitors for Cu10Ni alloy in sulfide-polluted salt water: Experimental and theoretical study, *Zastita Materijala*, 52(1), 21-35.
- [33] S.Rajendran, M.Kalpana Devi, A.Peter Pascal Regis, A.John Amalraj, J.Jeyasundari, M. Manivannan (2009) Electroplating using environmental friendly garlic extract, A case study, *Zastita Materijala*, 50(3), 131-140.
- [34] S. Rajendran, P. Chitradevi, S. Johnmary, A. Krishnaveni, S.Kanchana, Lydia Christy, R. Nagalakshmi, B. Narayanasamy (2010) Corrosion behaviour of SS 316 L in artificial saliva in presence of electrol, *Zastita Materijala*, 51(3), 149-158.
- [35] S.Rajendran, M.Agasta, R.Bama Devi, B.Shyamala Devi, K. Rajam, J.Jeyasundari (2009) Corrosion inhibition by an aqueous extract of Henna leaves (*Lawsonia Inermis L*), *Zastita Materijala*, 50(2), 77-84.
- [36] A. Christy Catherine Mary, S. Rajendran, J. Jeyasundari (2017) Influence of Coffee on the corrosion resistance of SS 316L, Ni-Ti alloy and thermoactive alloy in artificial saliva, *Eur.Chem.Bull*, 6(6), 232-237.
- [37] V. Sribharathy, S. Rajendran, P. Rengan, R. Nagalakshmi (2013) Corrosion Inhibition By An Aqueous Extract Of Aleovera (L) *Burm F.(Liliaceae)*, *Eur.Chem.Bull.*, 2(7), 471-476.
- [38] R.Epshiba, A.Peter Pascal Regis, S.Rajendran (2014) Inhibition Of Corrosion Of Carbon Steel In A Well Water By Sodium Molybdate-Zn 2 System, *Int.J.NanoCorros.Sci and Engg.*, 1(1), 1-11.
- [39] N.Kavitha, P.Manjula (2014) Corrosion Inhibition of Water Hyacinth Leaves, Zn^{2+} and TSC on Mild Steel in neutral aqueous medium, *Int. J. NanoCorros.Sci and Engg.*, 1(1), 31 - 38.
- [40] R.Nagalakshmi, L.Nagarajan, R.Joseph Rathish, S.Santhana Prabha, N.Vijaya, J.Jeyasundari, S. Rajendran (2014) Corrosion Resistance Of SS316L In Artificial Urine In Presence Of D-Glucose, *Int.J.Nano Corros.Sci and Engg.*, 1(1), 39- 49.
- [41] J.Angelin Thangakani, S.Rajendran, J.Sathiabama, R.M.Joany, R.Joseph Rathis, S.Santhana Prabha (2014) Inhibition Of Corrosion Of Carbon Steel In Aqueous Solution Containing Low Chloride Ion By Glycine - Zn^{2+} System, *Int.J.Nano Corros.Sci and Engg.*, 1(1), 50 - 62.

IZVOD

OTPORNOST NA KOROZIJU LEGURE Ni-Ti, LEGURE SS18 / 8 I TERMOAKTIVNE LEGURE U VEŠTAČKOJ PLJUVAČCI U ODSUSTVU I PRISUSTVU ČAJA

Otpornost na koroziju legure Ni-Ti, legure SS18 / 8 i termoaktivne legure u veštačkoj pljuvački (AS) u odsustvu i prisustvu čaja procenjena je polarizacijom. Za legure Ni-Ti, legure SS18 / 8 i termoaktivne legure, polarizaciono ispitivanje dovodi do zaključka da se otpornost na koroziju legure Ni-Ti i termoaktivne legure smanjuje u redosledu

AS + Tea > Tea > AS

Stoga, ljudi implantirani sa ortodontskom žicom, napravljenom od legure Ni-Ti legure i termoaktivne legure mogu uzimati čaj oralno bez ikakvih oklevanja.

Za leguru SS18/8, studija polarizacije dovodi do zaključka da se otpornost na koroziju legure SS18 / 8 smanjuje u redosledu

AS > AS + Tea > Tea

Dakle, ljudi implantirani sa ortodontskom žicom, napravljenom od legure SS18/8 trebalo bi izbegavati uzimanje čaja.

Ključne reči: *otpornost na koroziju, ortodontska žica, veštačka pljuva, ekstrakt čaja, Ni-Ti legura, legura SS18/8, termoaktivna legura, polarizacija.*

Naučni rad

Rad primljen: 21.07.2017.

Rad korigovan: 07.09.2017.

Rad prihvaćen: 12.09.2017.

Rad je dostupan na sajtu: www.idk.org.rs/casopis